


Function Selection Tabs

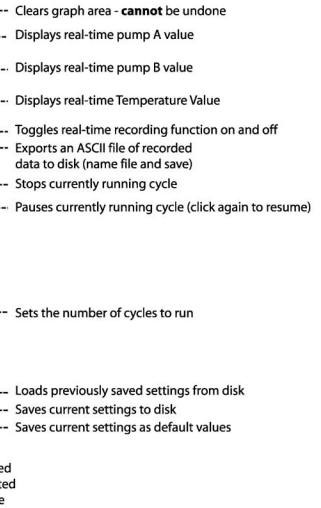


Select the type of value to be entered in flow rate value field.
Control value = either bit value sent to analog output or, after calibration, use convenient ml / min values

Resets flow rate value to factory default
Begins calibration procedure
(requires pump & graduated cylinder)

Enter volume of fluid pumped
in one minute when prompted
during calibration procedure

Function Selection Tabs

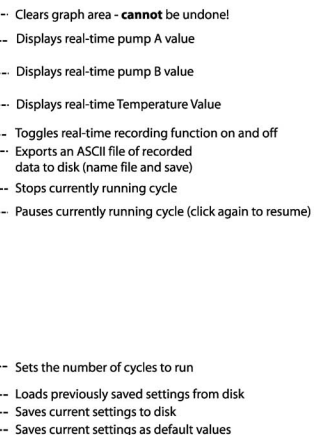

Voice: 724-282-7145 E-mail: info@bioptechs.com Web: www.bioptechs.com